

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re application of:

Lloyd Wolfinbarger, Jr.

Appl. No.: 08/646,520

Filed: May 7, 1996



Art Unit: 3306

Examiner: Blyveis, D.

Atty. Docket: 152.116P

#9

For: **A Recirculation Method for Cleaning
Essentially Intact Bone Grafts Using
Pressure Mediated Flow of Solutions
and Bone Grafts Produced Thereby**

DECLARATION UNDER RULE 1.131(a)

Commissioner of Patents and Trademarks
Washington, D.C. 20231

Dear Sir:

Dr. Lloyd Wolfinbarger, Jr., Phd., the applicant in the above-identified patent application, and Billy G. Anderson, president and CEO of LifeNet Research Foundation, the assignee, declare as follows:

1. That sometime prior to January 21, 1994, Dr. Lloyd Wolfinbarger, a research scientist, conceived of a method for cleaning intact bone grafts using negative or vacuum pressure to remove bone marrow and bone marrow elements from a bone graft;
2. That said method included subjecting the essentially intact bone graft including the internal matrix thereof to a vacuum mediated flow of solvent to remove bone marrow elements to produce a cell-free bone matrix;


3. That Dr. Lloyd Wolfinbarger successfully performed the method prior to January 21, 1994, as evidenced by Exhibit A attached hereto. Exhibit A includes (i) a copy of Dr. Wolfinbarger's dated (October 1, 1992) notebook page illustrating the method for cleaning bone using a vacuum mediated flow of solution; (ii) a copy of two pages dated March 1, 1993 showing the results obtained using the vacuum method to clean bone, the graph illustrating protein concentration versus detergent volume; and (iii) a copy of two photographs, front and back, dated "May 1993" on the back, illustrating bone being processed using the vacuum mediated method;
4. After successful performance of the method in 1993, LifeNet Research Foundation, the assignee of the present application optimized and perfected the method with Dr. Lloyd Wolfinbarger, and filed a patent application on February 27, 1995, issued on September 17, 1996 as U.S. patent no.: 5,556,379, which is the parent application of the present application, entitled: "Process for Cleaning Large Bone Grafts and Bone Grafts Produced Thereby" which is directed to cleaning bone using a vacuum mediated flow of solution;
5. After filing of the '379 patent application, Standard Operating Procedures (SOP's) were designed, as evidenced by Exhibit B attached hereto which includes a copy of two documents that are dated SOP's reflecting the vacuum mediated flow method of cleaning bone, that Billy G. Anderson President and CEO of LifeNet Research Foundation, on or about May 15, 1995, put into use as evidenced by

Exhibit B attached hereto which states that the method was instituted on May 15, 1995;

6. That Billy G. Anderson President and CEO of LifeNet Research Foundation, on or about May 29, 1996 put the present negative pressure mediated recirculation method as recited in the SOP's attached hereto as Exhibit C into use as evidenced by Exhibit C which includes a copy of two documents which show the recirculation method and reflects an effective date of May 29, 1996 and an approval date of May 28, 1996 (document 163.002) and May 21, 1996 (document 034.005);


The declarants further state that the above statements were made with the knowledge that willful false statements and the like are punishable by fine and /or imprisonment, or both, under Section 1001 of Title 18 of the United States Code, and that any such willful false statement may jeopardize the validity of this application or any patent resulting therefrom.

Mr. Billy G. Anderson, President and CEO



Date: 11-7-97

Dr. Lloyd Wolfinbarger, Jr., Phd.




Date: 11/7/97

EXHIBIT A

Paravivide Processing of Bone

10/1/92

I. Focus on femur heads, proximal femurs, distal femurs.




Post-It [®] brand fax transmittal memo 7671		# of pages = 7
To: Bill	From: [Signature]	
Co.	Co.	
Dept.	Phone #	
Fax #	Fax #	


II. Flushing protocols



- 1) Flush @ varying volume of paravivide
 - 2) Flush @ H_2O_2 (varying volume)
 - 3) Flush @ H_2O (varying volume)
 - 4) etc.
- } temp. ?
45°C



(Vacuum)




VACUUM


- Objectives:
- Use Paravivide to "solubilize" the bone marrow tissue; varying volumes may be necessary to effectively solubilize the bone marrow tissue in the cancellous bone areas.
 - Use hydrogen peroxide to oxidize remaining tissue debris and create a positive pressure behind the solubilized bone marrow tissue to "force" it out of the cancellous bone.
 - Use water wash to flush paravivide & residual H_2O_2 from cancellous bone.
 - Options: use other detergent solutions i.e. 2% sodium dodecyl sulfate (an anionic detergent) etc.

Negative Pressure - AlloushTM


Position No.1 - 3/1/93 Flus
0.5 N NaOH solub., 37 deg., 17 hrs




Position No.2 - 3/1/93 Flush
0.5 N NaOH solub., 37 deg., 17 hrs



Position No.3 - 3/1/93 Flus
0.5 N NaOH solub., 37 deg., 17 hrs



Position No.4 - 3/1/93 Flus
0.5 N NaOH solub., 37 deg., 17 hrs




LIFENET
6809 WARD COURT
VIRGINIA BEACH, VA 23455


Negative Pressure - Allowash™

LIFENET
5809 WARD COURT
VIRGINIA BEACH, VA 23455

AVERAGE- 3/1/93 Flushing
0.5 N NaOH solub., 37 deg., 17 hrs




AVERAGE- 3/1/93 Flushing
0.5 N NaOH solub., 37 deg., 17 hrs





Allowayth Negative Person

LIFENET
5809 WARD COURT
VIRGINIA BEACH, VA 23455




may 93



AllowashTM - Negative Pressure

LIFENET
5800 WARD COURT
VIRGINIA BEACH, VA 23455



MAY 93

EXHIBIT B



US005556379A

United States Patent [19]**Wolfinbarger**[11] **Patent Number:** 5,556,379[45] **Date of Patent:** Sep. 17, 1996[54] **PROCESS FOR CLEANING LARGE BONE GRAFTS AND BONE GRAFTS PRODUCED THEREBY**[75] **Inventor:** Lloyd Wolfinbarger, Norfolk, Va.[73] **Assignee:** Lifenet Research Foundation, Virginia Beach, Va.[21] **Appl. No.:** 395,113[22] **Filed:** Feb. 27, 1995**Related U.S. Application Data**

[63] Continuation-in-part of Ser. No. 293,206, Aug. 19, 1994, abandoned.

[51] **Int. Cl.⁶** A61M 31/00[52] **U.S. Cl.** 604/49; 128/898; 623/16[58] **Field of Search** 128/898; 604/28, 604/48, 49; 600/36; 623/16; 435/1, 267, 268[56] **References Cited****U.S. PATENT DOCUMENTS**

4,020,183 4/1977 Asculai et al. .
 4,169,123 9/1979 Moore et al. .
 4,207,689 6/1980 Romera-Sierra et al. .
 4,258,722 3/1981 Sessions et al. .
 4,315,919 2/1982 Shanbrom .
 4,366,822 1/1983 Altshuler .
 4,412,985 11/1983 Shanbrom .
 4,456,589 6/1984 Holman et al. .
 4,526,751 7/1985 Gartner .
 4,553,974 11/1985 Dewanjee .
 4,637,931 1/1987 Schmitz .
 4,678,470 7/1987 Nashef et al. .
 4,695,536 9/1987 Lindstrom et al. .
 4,801,299 1/1989 Brendel et al. .
 4,891,221 1/1990 Shanborm .
 4,923,677 5/1990 Simon et al. .
 4,946,792 8/1990 O'Leary .
 4,975,526 12/1990 Kuberasampath et al. .
 4,994,030 2/1991 Glowczwaki Jr. et al. .
 5,037,437 8/1991 Matsen, III .
 5,041,055 8/1991 Roth .

5,047,030 9/1991 Draenert .
 5,106,626 4/1992 Parsons et al. .
 5,118,512 6/1992 O'Leary et al. .
 5,120,656 6/1992 O'Leary et al. .
 5,133,756 7/1992 Bauer et al. .
 5,167,961 12/1992 Lussi et al. .
 5,186,945 2/1993 Shanbrom .
 5,192,282 3/1993 Draenert 606/65
 5,333,626 8/1994 Morse et al. .
 5,454,815 10/1995 Geisser et al. 606/85

FOREIGN PATENT DOCUMENTS

952189 8/1982 U.S.S.R. .
 964545 7/1964 United Kingdom .

OTHER PUBLICATIONS

Helenius, A. et al. "Solubilization of Membranes by Detergents," *Biochim. Biophys. Acta* 415 (1975).


(List continued on next page.)

Primary Examiner—Randall L. Green*Assistant Examiner*—V. Alexander*Attorney, Agent, or Firm*—Klima & Hopkins, P.C.

[57]

ABSTRACT

A process for removing substantially all bone marrow from a large bone and a bone graft produced thereby. A large substantially intact bone is selected and excess cartilage is removed from at least one articulating surface of the bone. An opening is prepared through the cortical layer of the bone to permit access of a vacuum line to the bone cavity. A vacuum line is attached to the bone via the opening for application of vacuum to the bone cavity, and the opening is sealed. A vacuum is applied to draw a first cleaning solution through the bone cavity so as to draw the first solution and solubilized bone marrow through the vacuum line to exit the bone at the opening. The vacuum is discontinued when the bone has been substantially cleaned of bone marrow. Subsequently, a second flushing solution may be drawn through the bone cavity via vacuum.

58 Claims, 6 Drawing Sheets

*MAINTENANCE fee
 schedule:*

1st - 9.17.2000

2nd - 9.17.2004

3rd - 9.17.2008


EXHIBIT C

Confidential
Do Not Duplicate

CONFIDENTIAL

22

Allowash™ (Vacuum Intercalary Grafts) Instituted 5/15/95

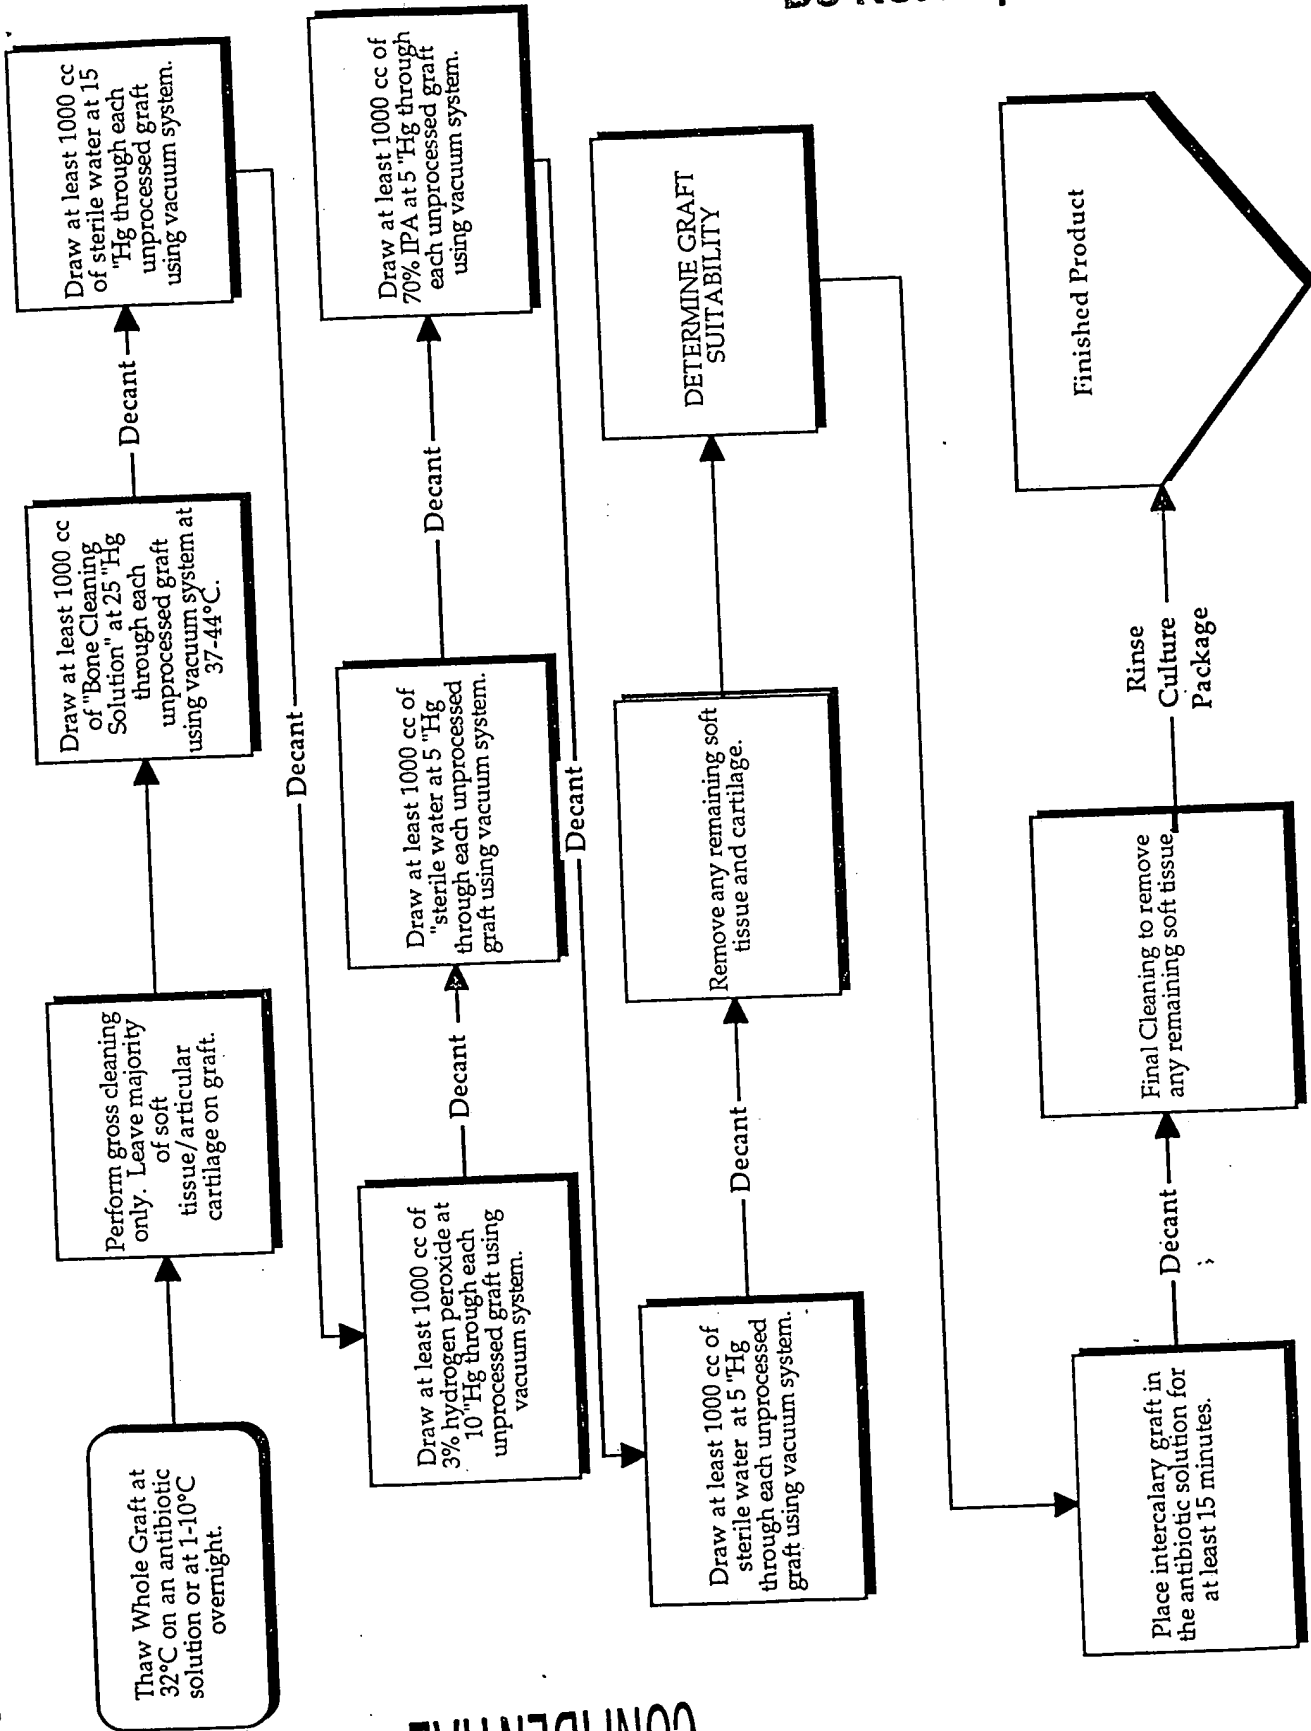

TITLE: PROCESSING FROZEN PROXIMAL FEMORA

Supersedes: PRO-MS-033.002		Written by: BB		Effective Date:	
Dept. Approval:		Division Approval:		QA Approval:	
Distribution	VP TP Svc	VP Tissue Svcs	VP Corp Svcs	MS	CV
				SPD	QA PTB SS
Annual QA Review:					

REFERENCES: MUSCULOSKELETAL TISSUE PROCESSING TRAYS, PRO-MS-060,
PRO-MS-064

PROCEDURE:

- A. Remove some of the soft tissue and periosteum from the graft material using sharp dissection techniques and periosteal elevators. **DO NOT REMOVE THE SOFT TISSUE BETWEEN THE FEMORAL HEAD AND GREATER TROCHANTER. THE ENTIRE LIGAMENT MUST BE REMOVED FROM THE FEMORAL HEAD FOVEA.**
- B. Transect the graft to no more than 22cm in length using a Stryker® saw or band saw. Ensure the cut is straight and contains no bone fragments. Remove all the muscle and periosteum approximately 2" proximal to the cut end.
- C. Remove the surface cartilage from the femoral head with either a scalpel blade, elevator, or osteotome.
- D. Using a 3/8" drill bit approximately 6" long, remove the contents of the intramedullary canal.
- E. Connect the intercalary vacuum apparatus to the cut end of the graft. Wrapping a cut end of the graft with a latex strip prior to attaching the intercalary vacuum apparatus may enhance the connection. Use only enough stripping to ensure a tight seal.

Confidential
Do Not Duplicate

- F. Connect an O-clamp to the intercalary apparatus/latex/ and graft junction and tighten. Connect a 1/2" vacuum line to one of the intercalary apparatus. To further enhance the connection, another latex strip and Parafilm® may be wrapped around the junction of the intercalary apparatus and graft.
- G. Connect the 1/2" vacuum tubing from the intercalary apparatus to a port on the sterile vacuum manifold. The vacuum manifold is attached to the collection canister at the "Ortho" port using 1/2" vacuum tubing. A 3/16" vacuum line is then attached to the vacuum pump from the collection canister.

Cap all unused ports on the vacuum manifold prior to turning the vacuum pump on.

- H. Place the graft and intercalary vacuum apparatus set-up in a deep sterile basin.
- I. Pour approximately 6000cc of a 1:100 dilution of Osteoclenz™ into the deep sterile basin. The Osteoclenz™ dilution is prepared by adding 6cc of 10x Osteoclenz™ to 5994 cc of sterile water. Ensure the basin is clearly labeled as "Osteoclenz™."

The temperature of the solution must be between 37° and 44° C. Place the deep sterile pan on a warmer if necessary. Each of the grafts must remain immersed in fluids at all times.

- J. Critical Step: Set the vacuum pressure to 25 in.Hg and draw the Osteoclenz™ through the graft(s). At least 1L of Osteoclenz™ must be infused through each allograft. Record the vacuum pressure, volume of infused solution and temperature of the Osteoclenz™ on the "Tissue Processing Log Worksheet."

Periodically inspect the vacuum lines. Any large bubbles indicate a leak in the vacuum tubing set-up. Tighten the O-Ring, reapply the latex stripping, or add Parafilm® to secure the seal.

Confidential
Do Not Duplicate

- K. Critical Step: Decant any remaining 1:100 dilution of Osteoclenz™ solution and add approximately 6L of sterile water to the deep sterile basin. Ensure the basin is clearly labeled as "Sterile Water." Draw at least 1L of water through the graft at 15 in.Hg. Record the vacuum pressure, volume of infused solution and exposure time on the "Tissue Processing Log Worksheet."
- L. Critical Step: Decant any remaining sterile water and add approximately 6L of 3% hydrogen peroxide to the deep sterile basin. Ensure the basin is clearly labeled as "Hydrogen Peroxide." Draw at least 1L of 3% hydrogen peroxide through the graft at 10 in.Hg. Record the vacuum pressure, volume of infused solution and exposure time on the "Tissue Processing Log Worksheet."
- M. Critical Step.: Decant any remaining 3% hydrogen peroxide and add approximately 6L of sterile water to the deep sterile basin. Ensure the basin is clearly labeled as "Sterile Water." Draw at least 1L of sterile water through the graft at 5 in.Hg. Record the vacuum pressure, volume of infused solution and exposure time on the "Tissue Processing Log Worksheet."
- N. Decant any remaining sterile water and add approximately 6L of 70% isopropyl alcohol to the deep sterile basin. Ensure the basin is clearly labeled as "70% IPA." Draw at least 1L of 70% isopropyl alcohol through the graft at 5 in.Hg. Record the vacuum pressure, volume of infused solution and exposure time on the "Tissue Processing Log Worksheet."
- O. Critical Step.: Decant any remaining 70% isopropyl alcohol and add 3L of sterile water to the deep sterile basin. Ensure the basin is clearly labeled as "Sterile Water." Draw at least 1L of sterile water through the graft at 5 in.Hg. Record the vacuum pressure, volume of infused solution and exposure time on the "Tissue Processing Log Worksheet."

TITLE: PROCESSING FROZEN PROXIMAL FEMORA

P. Remove the remaining soft tissue and cartilage and place the graft(s) in a basin with the antibiotic solution for at least 15 minutes. Ensure the basin is clearly labeled as "Antibiotics." Record the exposure time to the antibiotics on the "Tissue Processing Log Worksheet."

Q. Remove any remaining soft tissue if necessary and rinse again before culturing.

If the sterile wire wheel is used to remove the remaining soft tissue, ensure the Lucite™ capture box is surrounding the graft to minimize soft tissue discharge.

R. Assign the graft(s) the appropriate identification number, record the measurements on the processing log worksheet (record the condyle width, side, and total graft length), and culture the fashioned graft(s) for bacterial contamination with sterile cotton-tipped applicators. Place one cotton-tipped applicator into a TGC tube, and one into a TSB tube, label with the graft identification number. Refer to PRO-MS-060.

S. The graft material is now ready for packaging and placement in the appropriate freezer. Refer to PRO-MS-064. The graft must be x-rayed if requested.

CONFIDENTIAL

Allowash™ Treated Frozen Intercalary Tissue/Positive Pressure

Frozen Proximal Tibia
Frozen Proximal Humerus
Frozen Proximal Femur with Head
Frozen Proximal Femur
Frozen Distal Femur

Confidential
Do Not Duplicate

EXHIBIT D

CONFIDENTIAL


PAGE 1 OF 1

DOCUMENT#: PRO-MS-163.002

TITLE: ALLOWASH™ INTERCALARY GRAFT FLOW DIAGRAM

Supersedes: PRO-MS-163.001	Written by: BB	Effective Date: MAY 29 1996
Dept. Approval: BB 5/28/96	Division Approval: BB 5/28/96	QA Approval:
Distribution:	VP TP Svcs	VP Tissue Svcs
	VP Corp Svcs	MS
	CV	SPD
	QA	SS
Annual QA Review:		

REFERENCES: PRO-MS-036, PRO-MS-035, PRO-MS-034, PRO-MS-033, PRO-MS-028

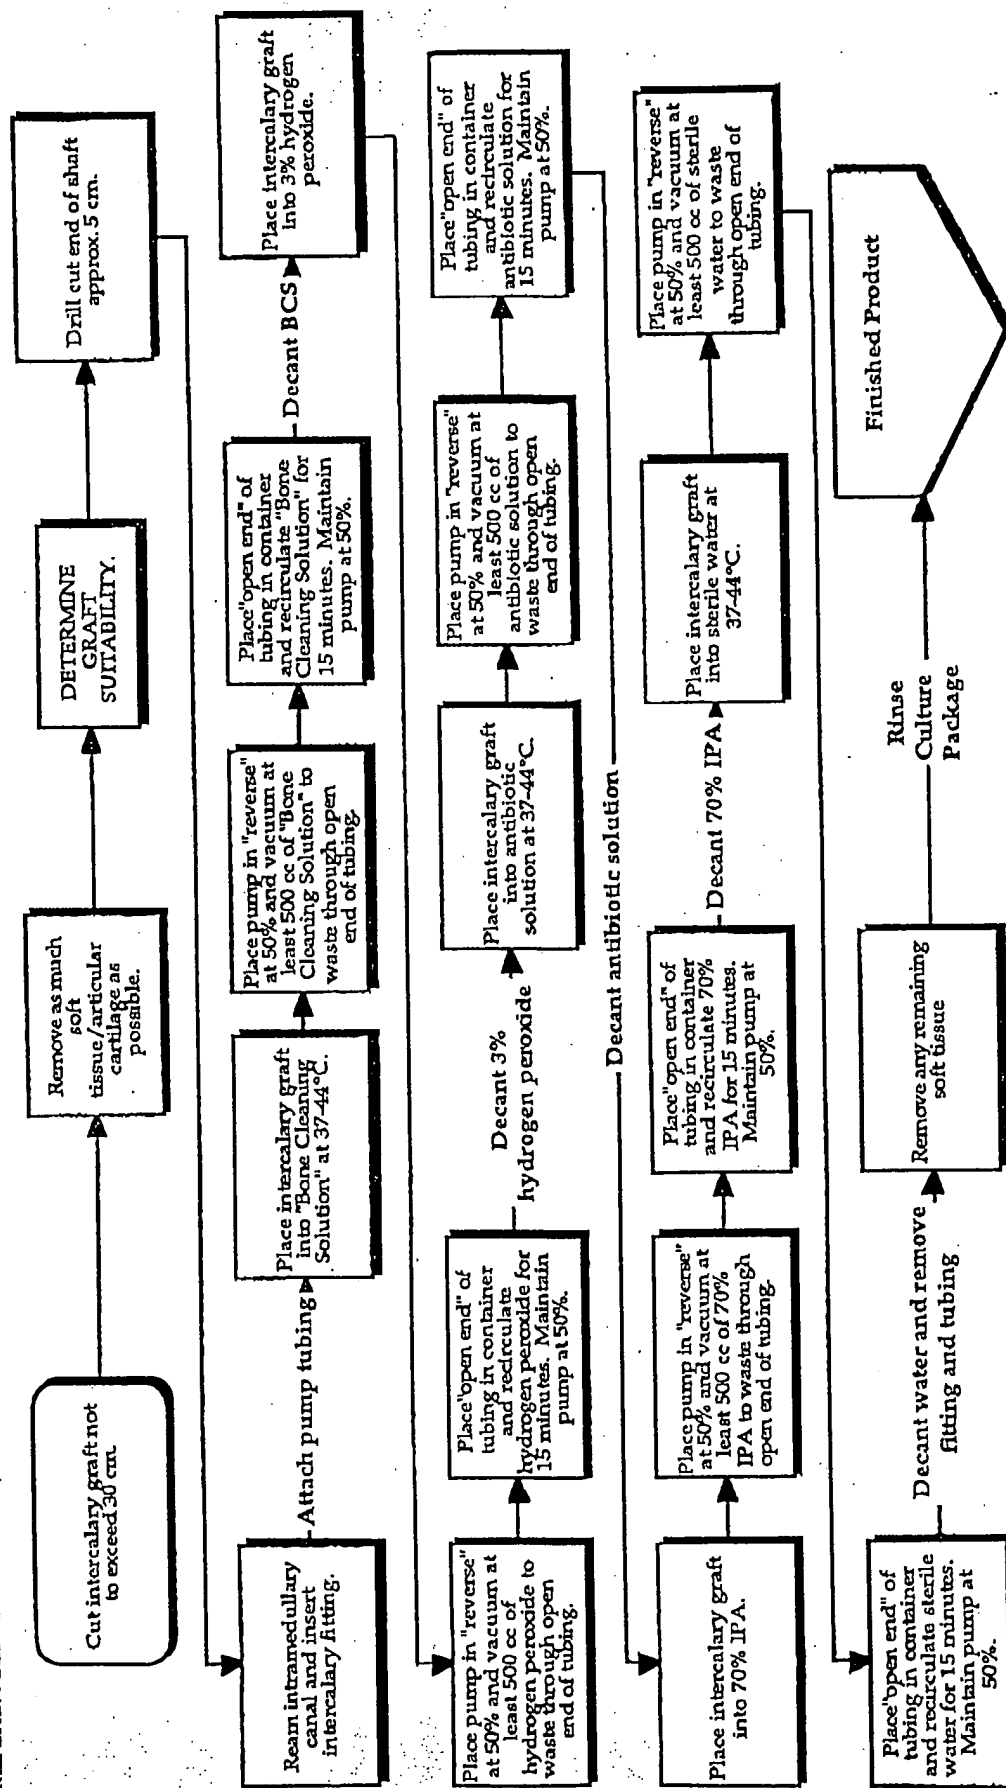

Supercodes: PRO-MS-034.004	Written by: CKW,AH	Effective Date: May 29, 1996
Dept. Approval: ED 5/31/96	Division Approval: SS 5/23/96	QA Approval: LA 5/23/96
Distribution: VP TP Svc VP Tissue Svcs VP Corp Svcs MS CV SPD QA SS		
Annual QA Review:		

Sup
(5/28/96)

REFERENCES: PRO-MS-010, PRO-MS-060, PRO-MS-064, PRO-MS-136

PROCEDURE:

- A. Transect the graft to the desired length using a Stryker® saw or band saw. Ensure each bisected piece is not more than 30 cm in length. Ensure the cut is straight and contains no bone fragments.
- B. Remove all of the soft tissue and periosteum from the graft material using sharp dissection techniques and periosteal elevators.
- C. Remove the surface cartilage from the femoral head with either a scalpel blade, periosteal elevator, or osteotome. The processing instructions may dictate leaving the cartilage "on" when appropriate.
- D. Using a 3/8" drill bit, drill the cut end of the shaft approximately 5 cm. Thoroughly wash the interior of the intramedullary canal with the lavage system.
- E. Insert the intercalary fitting by screwing the threaded, tapered end into the cut end of the graft.
- F. Assemble the vacuum tubing by securing one end of the tubing to the nipple end of the intercalary fitting. Secure the other end of the tubing to the piston driven pump. Finally, secure another section of vacuum tubing to the other side of the piston pump.

- G. Pour approximately 4000 cc of a 1:100 dilution of the "Bone Cleaning Solution" into the sterile flushing vessel. The "Bone Cleaning Solution" is prepared by adding 4 cc of cleaning reagent to 3996 cc of sterile water. Refer to PRO-MS-136. Ensure the flushing vessel is clearly labeled as "Bone Cleaning Solution".

The temperature of the "Bone Cleaning Solution" solution must be between 37° and 44° C.

- H. Critical step: Place the "open" end of the second piece of vacuum tubing into a graduated Fleaker™ flask. Set the piston pump to "reverse" and set the flow rate controller to 50%. Turn on the pump and vacuum at least 500 cc of the "Bone Cleaning Solution" to waste. Record the vacuum times, the approximate volume of solution, and the flow rate controller setting on the "Tissue Processing Log Worksheet". Do not allow the level of fluid in the column to fall below the intercalary fitting.
- I. Critical step: Remove the "open" end of the second piece of vacuum tubing from the graduated Fleaker™ flask and place it into the sterile flushing vessel. Maintain the drive in the "reverse" position at 50%. Allow the "Bone Cleaning Solution" to recirculate for a minimum of 15 minutes. Record the temperature, exposure time, and flow rate controller setting on the "Tissue Processing Log Worksheet."
- J. Critical step: Decant the 1:100 dilution of the "Bone Cleaning Solution" and add approximately 4L of 3% hydrogen peroxide to the flushing vessel. Set the piston pump to "reverse" and set the flow rate controller to 50%. Turn on the pump and vacuum at least 500 cc of the 3% hydrogen peroxide solution to waste. Record vacuum time, approximate volume of discarded solution, and the flow rate controller setting on the "Tissue Processing Log Worksheet". Do not allow the level of fluid in the column to fall below the intercalary fitting.

- K. Critical step: Remove the "open" end of the second piece of vacuum tubing from the graduated Fleaker™ flask and place it into the sterile flushing vessel. Maintain the flow rate controller in the "reverse" position at 50%. Allow the hydrogen peroxide to recirculate for a minimum of 15 minutes. Ensure the flushing vessel is clearly labeled as "3% Hydrogen Peroxide". Record the exposure time and the flow rate controller setting on the "Tissue Processing Log Worksheet."
- L. Critical step: Decant the hydrogen peroxide and add approximately 3980 cc of sterile water and the entire reconstituted vials of Bacitracin and Polymyxin B to the flushing vessel. Refer to PRO-MS-010. Ensure the flushing vessel is clearly labeled as "Antibiotic." Set the piston pump to "reverse" and set the flow rate controller to 50%. Turn on the pump and vacuum at least 500 cc of antibiotic solution to waste. Record vacuum time, approximate volume of discarded solution, and the flow rate controller setting on the "Tissue Processing Log Worksheet". Do not allow the level of fluid in the column to fall below the intercalary fitting.

The temperature of the water/antibiotic solution must be between 37° and 44° C.

- M. Critical step: Remove the "open" end of the second piece of vacuum tubing from the graduated Fleaker™ flask and place it into the sterile flushing vessel. Maintain the drive in the "reverse" position at 50%. Allow the antibiotic solution to recirculate for a minimum of 15 minutes. Record the temperature of the antibiotic solution, exposure time, and flow rate controller setting on the "Tissue Processing Log Worksheet."

DOCUMENT# PRO-M 4.005

CONFIDENTIAL

PAGE 4 OF 5

TITLE: PROCESSING FROZEN PROX. FEMORA WITH HEAD

- N. Critical step: Decant the antibiotic solution and add approximately 4L of 70% isopropyl alcohol to the flushing vessel. Ensure the flushing vessel is clearly labeled as "70% IPA." Set the piston pump to "reverse" and set the flow rate controller to 50%. Turn on the pump and vacuum at least 500 cc of 70% IPA to waste. Record vacuum time, approximate volume of discarded solution, and the flow rate controller setting on the "Tissue Processing Log Worksheet". Do not allow the level of fluid in the column to fall below the intercalary fitting.
- O. Critical step: Remove the "open" end of the second piece of vacuum tubing from the graduated Fleaker™ flask and place it into the sterile flushing vessel. Maintain the drive in the "reverse" position at 50%. Allow the IPA to recirculate for a minimum of 15 minutes. Record the exposure time and the flow rate controller setting on the "Tissue Processing Log Worksheet."
- P. Critical step: Decant the 70% isopropyl alcohol and add 4L of sterile water to the flushing vessel. Ensure the flushing vessel is clearly labeled as "Sterile Water." Set the piston pump to "reverse" and set the flow rate controller to 50%. Turn on the pump and vacuum at least 500 cc of sterile water to waste. Record vacuum time, approximate volume of discarded solution, and the flow rate controller setting on the "Tissue Processing Log Worksheet". Do not allow the level of fluid in the column to fall below the intercalary fitting.

The temperature of the sterile water must be between 37° and 44° C.

- Q. Critical step: Remove the "open" end of the second piece of vacuum tubing from the graduated Fleaker™ flask and place it into the sterile flushing vessel. Maintain the drive in the "reverse" position at 50%. Allow the water to recirculate for a minimum of 15 minutes. Record the temperature of the water, exposure time, and the flow rate controller setting on the "Tissue Processing Log Worksheet."
- R. Disconnect the tubing and remove the intercalary fitting from the graft.

S. Remove any remaining soft tissue if necessary and rinse again before culturing.

If the sterile wire wheel is used to remove the remaining soft tissue, ensure the Lucite™ capture box is surrounding the graft to minimize soft tissue discharge.

T. Assign the graft the appropriate identification number, record the measurements on the processing log worksheet (record the side (R/L), femoral head size, and total graft length). Culture the fashioned graft for bacterial contamination with sterile cotton-tipped applicators. Place one cotton-tipped applicator into a TGC tube, and one into a TSB tube, label with the graft identification number. Refer to PRO-MS-060.

U. The graft material is now ready for packaging and placement in the appropriate freezer. Refer to PRO-MS-064. The graft must be x-rayed if requested.